
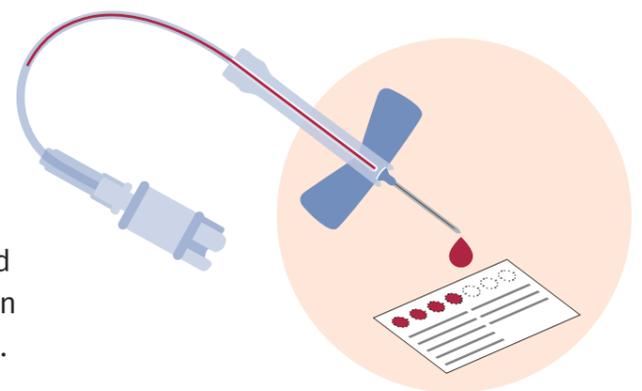


Newborn Screening Bloodspot Collection

GUIDELINE

1a Blood collection from the heel (newborns)


- Clean the heel and disinfect with alcohol or isopropanol, if necessary. Do not use any disinfectant.
- If required, massage or warm the heel, use commercially available lancing devices (safety lancets with a wide cutting surface).
- Puncture the heel laterally and wipe off the first drop of blood with a clean swab.
- Apply blood onto the pre-printed filter paper circles, without touching the card with the heel.
- Fill 2 - 7 circles fully, depending on the analysis requested.
- For newborn screening 5 or more circles must be filled completely.

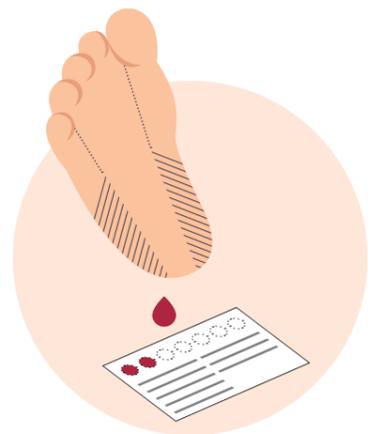

1b Alternatively: venous blood collection

Only qualified medical professionals may carry out venous blood collection. Hygiene and medical instructions must be strictly adhered to. Apply blood directly from the collection system onto the dried blood card or use a pipette to transfer it from the collection tube. Do not use any additives (EDTA, heparin, etc.).

Caution: Apply a large drop of blood onto each circle to ensure the circles are filled as completely as possible. The blood must soak through the card so that blood spots look almost equal on both sides. Apply blood onto the card from one direction only. Avoid multiple blood applications (overloading). Do not use umbilical cord blood! Do not draw blood from intravenous catheters!

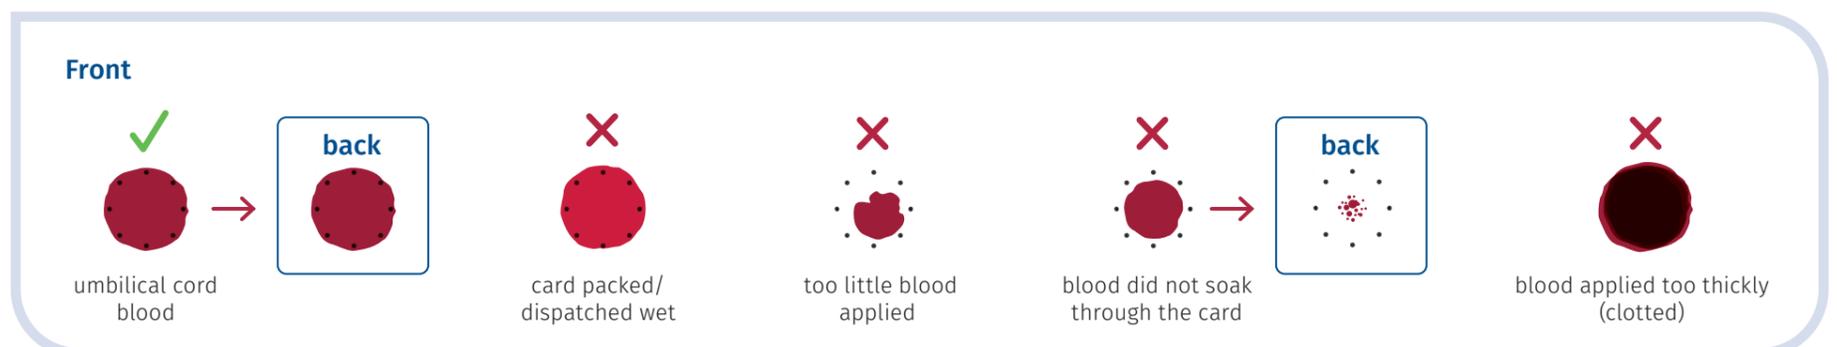

2 Drying

Allow to dry at room temperature for at least 2 - 4 hours by placing the card upright/inclined against an object. Do not dry the card with a radiator, a hairdryer or with exposure to sunlight!



3 Preparation for shipment

- Fill out data fields on request form and dried blood card completely.
- Check parental consent for valid signatures. This remains in the patient's medical record and a copy given to parents.
- Put the request form, dried blood card and, if required, laboratory referral letter in an envelope, stamp sufficiently and send as soon as possible.
- Avoid mailboxes exposed to strong sunlight or cold, consider date and time of postal collection. Sending from a post office or centre is recommended.

Blutropfen:
Beste Qualität erforderlich!
Mindestens 5 Kreise von dieser Seite her mit jeweils 1 großen Tropfen Blut vollständig durchtränken.
Kein EDTA!

Blood spots:
Best quality essential!
Fill at least 5 circles completely with one single very large drop of blood each from this side only.
No EDTA!

Name
Vorname
First name
Geburtsdatum
Date of birth
Datum Blutentnahme
Date of blood collection

Einsender: Stempel oder Aufkleber
Sender: stamp or label



Screening-Labor Hannover
P.O. Box 91 10 09
30430 Hanover
Fon: 05108-92163-0
Fax: 05108-92163-19

Copyright 2020 – All contents, especially text, pictures and graphics are governed by the copyright laws of Germany. Any duplication, processing, distribution, transaltion or any form of utilisation beyond the scope of copyright law shall require the prior written consent of the Screening-Labor Hannover. For questions or additional information, please contact the laboratory.

Design: NF.DESIGN / Nina Fischer